

# Operator's Handbook

## for

### Compact

### High Voltage

### P20 & P40

## POROSITY (HOLIDAY) DETECTORS



**Can be used in accordance with:  
Australian Standard AS3894.1**

ASTM G62, ASTM D5162, ASTM D4787, NACE SP0274,  
NACE TM0186, NACE TM0384, NACE SP0490,  
NACE SP0188, ANSI/AWWA C214, ISO 29601



CE Marked PCWI Compact Detectors comply with the requirements of  
EMC Directives 89/336/EEC EMC and its amending directives.

## **POROSITY DETECTOR ACCURACY:**

±%3% above 10kv ±10% below 10kV

Note: at the time PCWI tested the Porosity Detector at the reference temperature & humidity).

Refer to the PCWI Manufacturer's Calibration Certificate provided with the Porosity Detector.

Recertification available



## WARNING

Unlike continuous direct current units where the electrical field drops to zero when contact is made and where the probe is earthed out via the body, **Pulsed Detectors will continue to shock at full voltage.** Caution should be taken to avoid contact with the live electrode.

## CONTENTS

1.0 Safety Precautions	4
2.0 Operation	5
3.0 Specifications	6
4.0 Control Panel Layout	7
5.0 Voltage Recommendations	8-9
6.0 Troubleshooting	10-11
7.0 Optional Detector Accessories	12-13
8.0 PCWI NiMH Battery Charger & Clip	14-15
9.0 Warranty	16
10.0 Service & Maintenance	17

## INTRODUCTION

Thank you for choosing the PCWI Compact for pre-installation and post installation corrosion detection.

PCWI have designed this instrument with care, to provide ongoing corrosion detection efficiency under a wide variety of coating application conditions and to ascertain Porosity for the many protective coatings currently in use. Under reasonable care in operation, the unit will provide many years of trouble free detection.

To support the unit, PCWI maintain a comprehensive range of Electrodes (probes) - extending the versatility of the Compact from large to small and from accessible to inaccessible surfaces.

PCWI, in a continuing desire to achieve the maximum in corrosion detection competence, welcomes user enquiries and recommendations.

Yours sincerely



Paul Van Gaal



## 1.0 SAFETY PRECAUTIONS:

All hand-held high voltage test equipment should be operated by responsible, trained and authorised personnel.

**The unit must be earthed to both the item under test and to ground.**



### CAUTION

The Detector output can be up to 40,000 volts. Should the operator accidentally make contact with the test electrode, they may experience a mild shock or zap, and in order to avoid this possibility, the wearing of rubber gloves is recommended.

Furthermore, the operator should enjoy good health and not suffer from a cardiac condition. **If the operator has a pacemaker, then they should not use this equipment.**

This equipment should only be used for the purpose for which it was designed, ie: checking the porosity, or electrical breakdown, of dielectric or insulating materials.

It is also recommended that testing should be carried out well clear of personnel not involved in the testing procedure, or in such a position whereby the surprise of receiving an electric shock could cause a related accident, if for example, tests being carried out close to moving or rotating machinery, or in such an unstable position that the operator could fall and injure themselves.

It is recommended that the operator should have an assistant, to ensure that unauthorised personnel are kept well clear of the testing area, and generally assist when necessary with the testing procedure. It is also recommended that the Detector not be operated within close proximity of sensitive electronic apparatus, such as computer equipment.

### DANGER

Do not use the test equipment in any combustible or flammable atmosphere, as a test voltage can cause an arc or spark to be generated and an explosion could result.

Always consult the plant or safety officer before carrying out a test procedure.

When testing tank internals, be certain the tank does not contain solvents remaining from the painting procedure.

## Coating Thickness Range

Applied coats should be cured, thickness tested, visually inspected and accepted – before high voltage porosity testing is carried out. Coating thickness should be above 150µm; coatings below this thickness should be tested with a wet sponge unit.

## 2.0 OPERATION

Connect the probe and earth leads to the unit. Connect the earth clamp to the metallic substrate of the item to be tested – substrate should be earthed to ground. Select the probe best suited for the test and attach to the probe handle.

Fit the Fuse (if not already fitted).

Turn the unit on.

Test the batteries to ensure that they are charged.

Adjust the voltage control to the required test voltage.

Place the probe near the metal substrate.

A spark should occur (if not re-check all leads and connections).

At the same time the operation of the alarm can be checked.

The unit should now be ready for use.

Re-check the output – adjust if necessary.

Place the probe on the coated surface and move at approximately one metre per four seconds.

### A fault is indicated by:

A spark at the probe – this can usually be seen and heard.

A light flashes on the front panel of the unit.

An audible sound – buzzer is mounted inside the unit.

**Note:** A definite flaw should be made in the coating and located with the designated test voltage, therefore proving that the unit is locating the type of fault you wish to find.

Probes must be kept in full contact with the surface, gaps in or between the probe and the coating may result in flaws going undetected.

Wire brushes, rubber and coil spring probes should all be kept in good condition.

Probes other than fine wire brushes may require higher voltages.

## Earthing

Where the item to be tested is not earthed to ground, a ground spike **must** be attached.

The unit should always be switched off before removing and re-positioning the earth lead. After the earth is repositioned, the probe should always be flashed on the substrate to prove a good contact has been made.

## 3.0 SPECIFICATIONS


	<b>P20</b>	<b>P40</b>
Unit weight:	2.2kg	2.2kg
Packed weight :	8.0kg	8.0kg
Display:	LCD	LCD
Voltage:	0 to 20kv	0 to 40kv
Resolution:	100v	100v
Alarm range:	2 to 20kV	5 to 40kV
Short circuit test current:	1.5mA max	
Power supply:		Gel Cell 3Ah Clip On
Dimensions:		260 x 160 x 70mm
Alarm:		Audible
Probe handle:		Rubber lead
Battery condition:		LED Indicator

Optional coils & brushes available: See accessories pages

## STORAGE:

The Detector should be stored in a dry place. Leads should not be wound tightly. Battery should be fully charged.

## 4.0 CONTROL PANEL LAYOUT

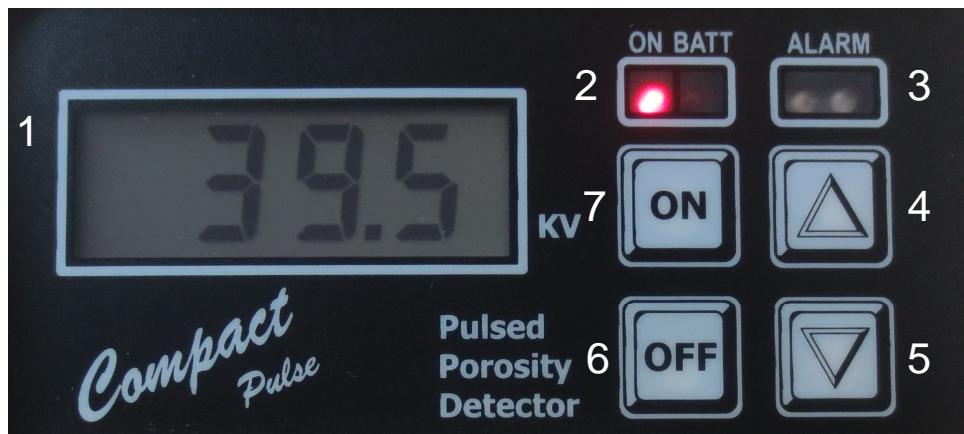

- 1 LCD display
- 2 On/Battery condition indicator Light
- 3 Visual alarm indicates when fault is found
- 4 Voltage Up
- 5 Voltage Down
- 6 Off
- 7 On
- 8 Audible alarm when fault is found
- 9 Earphone (connected on opposite side)
- 10 Pulse probe connection
- 11 Fuse (4A slow blow) 5 x 20mm
- 12 Earth connection point
- 13 Alarm sensitivity 'wet' or 'dry' conditions  
*(located in battery compartment)*
- 14 Slide-off power pack



Side view

## 5.0 VOLTAGE RECOMMENDATIONS

AS3894.1 recommends minimum voltages for testing specified thickness of film of various Coating Products

Tables 1 and 2 below provide guidance for determination of minimum voltage for high voltage porosity testing of the indicated generic types of coating products, at the indicated dry film thicknesses which may contain residual solvents.

**Table 1. Determination of the coating film rating (F) from coating type and volume solids content.**

Generic Type of Coating Volume Solids %(V/V)	Volume Solids %(V/V) Factor (F)	Factor (F)
Chorinated Rubber, Vinyl	15 to 39	4
Low Build Epoxy, some Tar Epoxy	40 to 59	3
High Build Epoxy, some Tar Epoxy	60 to 79	2
Polyester/Vinyl esters, Solventless Epoxy, Fusion-bonded Epoxy.	80 and greater	1

**Table 2. Determination of the test voltage (V) from dry film thickness (T) and coating material rating (F).**

Nominal dry film thickness in microns	Test Voltage (kV)			
	F=1	F=2	F=3	F=4
150	3.06	1.53	1.01	0.77
250	3.96	1.98	1.32	0.99
400	5.00	2.50	1.67	1.25
600	6.12	3.06	2.04	1.53
800	7.07	3.54	2.36	*
1500	9.69	4.84	*	*
2500	12.50	*	*	*
4000	15.81	*	*	*

Formula 1

$$V = \frac{250 \times \sqrt{T}}{F}$$

V = minimum test voltage applied in volts  
T = dry film thickness of cured coating in microns  
F = a whole number factor which rates a coating's generic type and residual solvent content (Table 1)

The above minimum test voltages have been derived from Australian Standard AS3894.1; the whole of this Standard should be used. The above voltages relate to the following: the detector should have a direct earth connection to the substrate and a fine wire brush electrode must be connected to the probe.

# International Standards

## NACE SP0274 derived table

Table 3 below is derived from NACE standards and should be used as a guide only.

Table 3. kV Values from NACE

mm	kiloVolts
0.51	6
0.79	7
1.6	10
2.4	12
3.2	14
4.0	16
4.8	17
13	28
16	31
19	34

The above table should be taken as a GUIDE only. It is recommended that the whole of this standard be used.

## 6.0 TROUBLESHOOTING

### Alarm Sensitivity Control

Located on the base of the **P20 & P40** compacts, underneath the battery pack, is an alarm sensitivity control switch.

This switch enables the operator to set the alarm sensitivity by selecting the most appropriate setting when working in conditions where the coating surface is wet.

The control “pot” can be adjusted to:

‘Dry’ For normal function in dry conditions

‘Wet’ For alarm function in wet conditions

<b>Symptom</b>	<b>Cause</b>	<b>Solution</b>
No Display	Flat battery	Recharge battery
	No power - fuse not fitted	Fit fuse
Alarm sounds continuously during test	Damp or wet surface	Set Alarm Sensitivity Control to 'Wet' (Control is located in battery compartment)
	Coating may not be fully cured	Allow coating to cure
	Probe moved too slow	Move probe 1 metre every 4 seconds
	Probe surface area too great	Use smaller probe
No spark at probe tip	Damaged leads	Repair or replace leads
	Poor connections	Clean and reconnect
	Flat battery	Recharge battery

## 7.0 OPTIONAL DETECTOR ACCESSORIES

### Crest Meter & Certification



### Brushes & Coils

50mm (2in) to 600mm (24in) wide flat brushes.

25mm (1in) to 500mm (20in) Spiral wound and Disc Internal circular pipeline brushes.

25mm (1in) to 500mm (20in) External circular pipeline brushes.

50mm (2in) to 1765mm (72in) Coils complete with ball bearing ends.



60mm, 125mm, 200mm, 450mm connectors for flat or external pipeline brushes.

Coil Joiners

Fan Brushes

Additional Accessories

Spare slip-out power packs.

7m Earth lead with clamp.

10m trailing Earth lead (1m plastic encased).

Spare neon light holders and neon's

**See [www.pcwi.com.au](http://www.pcwi.com.au) for more details**



## 8.0 PCWI NiMH Battery + Charger Clip BC-1

The BC-1 charging clip is for use with the PCWI NiMH Battery Pack and PCWI Charger PA-1015 Only.

Indicator Light Operation.

RED = Charging

GREEN = Charged

Flashing Red Green = Battery Conditioning.

**Note:** BC-1 and BC-1 V2 operate the same except for **BC-1 V2** Flashing Red Green continuously = No battery connected.

When battery is first placed into charging Clip the charge circuit will check the condition of the battery and the Green Indicator will illuminate.

If the battery is OK for charging the Indicator Light will change from Green to Red. It may take 5 to 10 seconds for the battery to be checked.

If the battery is defective or is less than 9 volts the Charge Indicator light will flash from Red to Green. During this time the charge circuitry will trickle charge the battery if possible.

The BC-1 Battery Clip will fast charge the battery to 75% of capacity in approximately 4 hours. The remaining 25% charge will occur in approximately 20 Hours.

If BC-1 Charge Clip is used with PCWI AC/DC Adapter Model No:- Select. A Part No:- SA48-1005 the battery will not be fast charged.



PCWI Battery Charging Clip with NiMH battery & power adaptors



PCWI NiMH battery Pack



NiMH Battery Pack Warning label

## 9.0 WARRANTY

Subject to the warranty conditions below this PCWI Instrument is warranted by PCWI International Pty Ltd to be free from defects arising from faulty design, material, or workmanship for a period of 12 months from the date of original purchase by the end user or a maximum period of 15 months from dispatch to authorised distributors. Probes and leads are warranted for 3 months. They are consumable items, and subject to wear and deterioration during use. The life of these parts can be much extended by keeping them in a dry clean condition, and storing them in suitable protective containers. During use, avoid "scrubbing" the probe along the surface of the work-piece.

## WARRANTY CONDITIONS

During the warranty period listed above PCWI or it's authorised service representative will make good any defects covered by this warranty. PCWI or it's authorised service representative will decide if there are any defects in design, material or workmanship. This warranty only applies provided the instrument has been used in accordance with the manufacturers operating handbook recommendations.

This warranty does not cover damage, malfunction or failure resulting from misuse, neglect, abuse or used for a purpose for which it was not designed and no repairs, alterations or modifications have been attempted by other than PCWI on an authorised service.

This warranty applies only to the original user buyer. This warranty does not cover any service that is needed after an accident, alterations, misuse, fire or floods.

This warranty is the only one given by PCWI and no one has the authority to change, or add to, the obligations and liabilities listed in it.

This warranty does not cover batteries, probe handle brushes (electrodes) and leads which are subject to wear.

During the warranty period PCWI or its authorised service representative will bear the transportation cost of the return of instrument/s repaired under warranty back to the users premises within the country of purchase.

## HOW TO MAKE A WARRANTY CLAIM

Defective goods must be returned to PCWI or an authorised service representative at the Purchaser's expense. The goods must be accompanied by the Purchaser's written order describing the defect and authorising PCWI or its authorized service representative to invoice the Purchaser for any charges not covered by the warranty.

The purchasers order must also include the model and serial numbers of the instrument and address of the distributor and date of purchase.

Upon receipt at the service point the instrument will be examined to determine the nature and cause of the defect.

If the defect is covered by the warranty, a repair will be effected at PCWI's or authorised service representative expense. If the defect is not covered by the warranty, PCWI or authorised service representative will quote the Purchaser for a replacement or repair, and will not proceed until written acceptance of the quotation is received.

## **10.0 SERVICE AND MAINTENANCE**

### **AUTHORISED SERVICE REPRESENTATIVE**

To enable speedy “return to service” whether under warranty or otherwise, PCWI have appointed your distributor as a service centre and have provided all relevant information and recommended parts to be carried to assist distributor’s technical staff carry out this essential part of the PCWI customer service.

### **CARE AND MAINTENANCE**

This equipment is protected against hostile environments and is designed for prolonged use in the field without any special maintenance, other than routine battery recharging. However, the equipment is not totally sealed and appropriate precautions should be taken. Remember, it is a precision electronic instrument and should be treated as such. There are no internal user controls.

The equipment should only be operated by qualified personnel.

Some organic materials may attack plastic parts and cause early degradation.

Contact with such materials should be avoided.

Do not operate damaged equipment.

Where the power supply is derived from internally mounted rechargeable cells and disassembly of the unit is necessary to access those batteries, this action would void all warranty.

### **SERVICE REPAIRS AND MAINTENANCE**

Repairs not covered by the warranty or carried out after the warranty period, will be charged at the current hourly or set service rate, plus the cost of materials.


Goods for repair must be sent at the Purchaser’s expense, and be accompanied by the Purchaser’s written order describing the defect and authorising PCWI to invoice the purchaser for labour, materials and return delivery cost.

No service or repair will be undertaken until a written order is received.

### **BEFORE YOU CALL FOR SERVICE**

Read the section on “troubleshooting” in this handbook and check the symptom, cause and solution before you call for service.

### **AUTHORISED SERVICE AGENT:**



## Notes:

# PCWI OFFERS

## **Strong technical support**

In-house development and manufacturing enables us to provide strong technical support and a quick response to enquiries and orders.

## **Market and product knowledge**

We understand technical specifications demanded by industry and recognise customer requirements are specific in relation to testing and measuring instruments.

## **Calibration laboratory**

PCWI's in-house laboratory supports testing for a range of instruments operating in accordance with ISO/IEC 17025. All certification is Traceable to National & International Standards of Measurement.

## **Quality systems certified to ISO9001**

PCWI's Quality Management System is certified to ISO9001 and audited by SAI Global.

## **Warranties and after sales service**

PCWI provides 12 months warranty for its Detectors with detailed operator instruction handbooks and after sales service. An extension of this PCWI service is provided by your local distributor.